

## Contacting Technical Support

For questions about installing or operating your Temperature/Humidity Sensor, please contact Davis Technical Support. We'll be glad to help.


Online	www.davisinstruments.com Find copies of user manuals, product specifications, application notes, software updates, and more.
E-Mail	support@davisinstruments.com
Telephone	(510) 732-7814 Monday - Friday, 7:00 A.M.- 5:30 P.M., Pacific Time

**Davis Instruments**® 3465 Diablo Ave., Hayward, CA 94545-2778 USA  
(510) 732-9229 • FAX (510) 670-0589 • www.davisinstruments.com

7395.361 Rev. A 2/11/2019

## Mounting your sensor


1. Unsnap the back plate from the sensor housing.

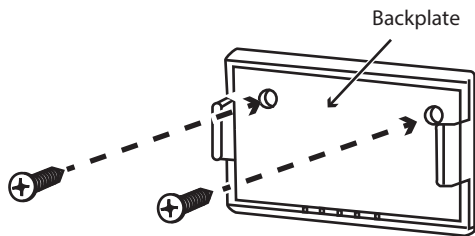

Using the backplate as a guide, mark and drill pilot holes where you want to install the sensor.

2. Use the two #6 screws included to install the backplate.
3. Snap the sensor onto the backplate.

4. *Optional:* If extra strain relief is needed, you may insert a #4 screw and washer into the strain relief portion of the sensor cable and secure to the surface.




5. Plug the RJ connector into the jack labeled "Temp/Hum" on a Sensor Transmitter (product numbers 6331 or 6332). (See the Sensor Transmitter User Guide.)

## Temperature/Humidity Sensor

Product number 6834

The Temperature/Humidity Sensor should be installed indoors.

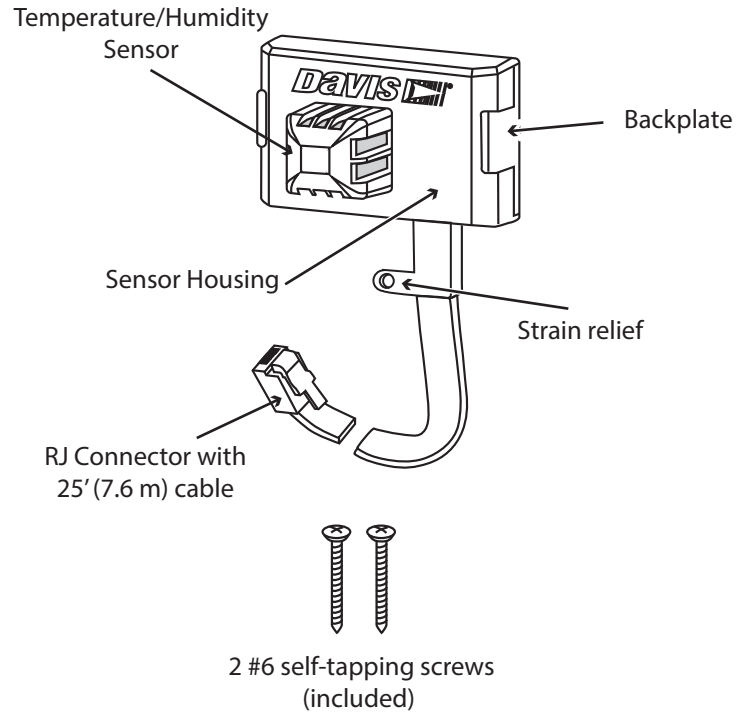

## Maintaining your sensor

To keep your Temperature/Humidity Sensor most accurate, you should inspect it periodically for dust, debris, and insect nests or webs. Clean the sensor screen with a soft brush.

## Sensor specifications

### Humidity

Resolution and Units	1%
Range	1 to 100% RA
Accuracy	±2%
Drift	<0.25% per year
Update Interval	50 seconds to 1 minute

### Temperature

Resolution and Units	0.1°F or 1°F or 0.1°C or 1°C (user-selectable)
Range	-40° to +150°F (-40° to +65°C)
Accuracy	±0.5°F (±0.3°C)
Update Interval	10 - 12 seconds